


```

=====
Acq. Operator   : 1
Acq. Instrument : Instrument 1                      Location : Vial 0
Injection Date  : 3/31/2018 11:09:29 AM
Acq. Method     : D:\CHEM32\
Last changed    : 3/31/2018 11:07:11 AM by 1
                  (modified after loading)
Analysis Method : D:\CHEM32\
Last changed    : 3/31/2018 10:30:36 AM by 1
                  (modified after loading)
Sample Info     : A = ACN, B = H2O] 10-95% A/B 3.5 min, 95% A/B 4.5 min,
                  95-10% A/B 1 min, 10% A/B 1 min; Athena C18 (3 µm, 2.1
                  mm × 100 mm); Flow: 0.5 ml/min, Temp = 50
    
```

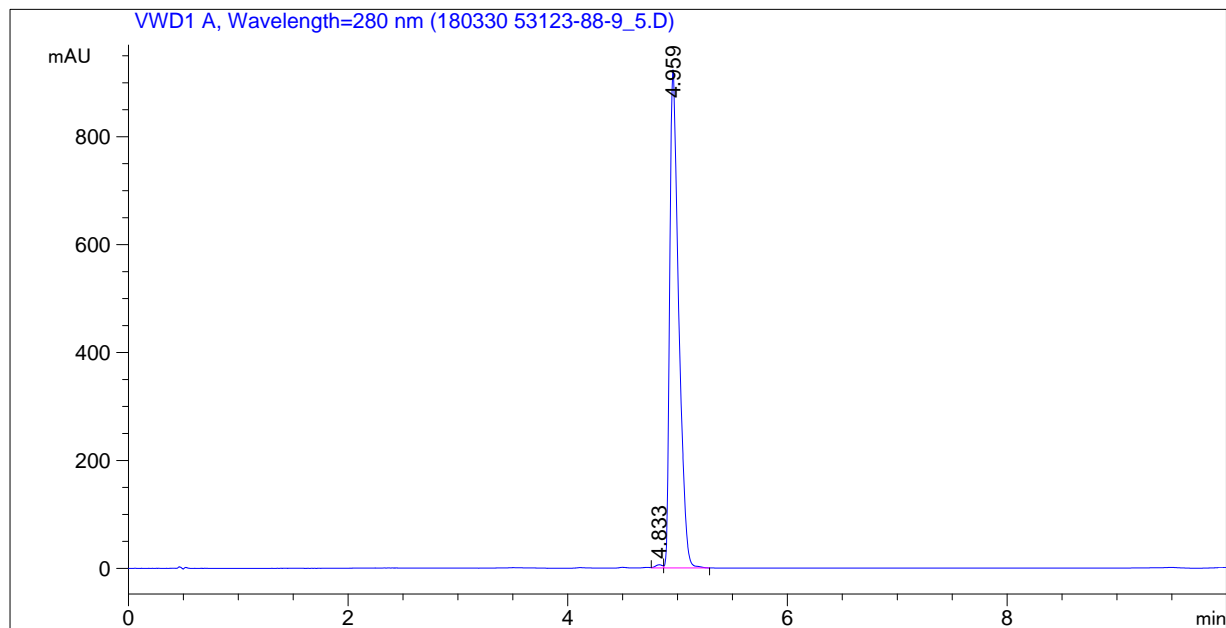

=====
 Area Percent Report
 =====

```

Sorted By      :      Signal
Multiplier:    :      1.0000
Dilution:      :      1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: VWD1 A, Wavelength=280 nm

Peak #	RetTime [min]	Type	Width [min]	Area mAU *s	Height [mAU]	Area %
1	4.833	VV	0.0686	25.54670	5.83463	0.4822
2	4.959	VB	0.0845	5271.94092	923.05762	99.5178
Totals :				5297.48762	928.89225	

=====
 *** End of Report ***